

Original scientific paper

An electrochemical sensing platform based on a modified carbon paste electrode with graphene/Co₃O₄ nanocomposite for sensitive propranolol determination

Parisa Karami-Kolmoti¹ and Reza Zaimbashi^{2*}

¹Department of Chemistry, Graduate University of Advanced Technology, Kerman, Iran

²Environment Department, Institute of Science and High Technology and Environmental Sciences, Graduate University of Advanced Technology, Kerman, Iran

*Corresponding Author: E-mail: r.zaim2017@gmail.com

Received: February 10, 2023; Revised: February 23, 2023; Published: March 15, 2023

Abstract

A simple and sensitive method for the determination of propranolol using a modified carbon paste electrode with graphene/Co₃O₄ nanocomposite was presented. The electrochemical measurements of propranolol are studied using differential pulse voltammetry, cyclic voltammetry and chronoamperometry. The graphene/Co₃O₄ nanocomposite exhibits excellent catalytic activity towards the electrochemical oxidation of propranolol in phosphate buffer solution of pH 7.0. The graphene/Co₃O₄ nanocomposite facilitates the determination of propranolol in the concentration range 1.0–300.0 μM and a detection limit and sensitivity of 0.3 μM. and 0.1275 μA/μM were achieved.

©2023 by the authors. This article is an open-access article distributed under the terms and conditions of the Creative Commons Attribution license (<http://creativecommons.org/licenses/by/4.0/>).

Keywords

Carbon paste electrodes; graphene/Co₃O₄ nanocomposite; differential pulse voltammetry; propranolol

Introduction

Propranolol (I) [1-(isopropylamino)-3-(1-naphthoxy)-2-propanol] is a highly effective and non-selective adrenergic receptor (-blocker) that is widely used in clinical practices to treat cardiovascular disorders, such as angina pectoris, arrhythmia, myocardial infarction, dysfunctional labor and anxiety. It possesses no autonomous nervous system activity and is completely absorbed from the gastrointestinal tract in healthy volunteers after oral administration. It affects the regulation of blood circulation by reducing the cardiac frequency, myocardial contractility, contraction force, coronary flow and secretion of rennin, resulting in a fall in the level of angiotensin II, which contributes significantly to the hypertensive action of this drug. It also lowers blood pressure by altering the transmission of nerve impulses from the brain to a certain part of the body and causes relaxation (and possibly dilation) of blood vessels, decreasing heart rate and pulse. Propranolol has been listed as a banned substance by World Anti-Doping Agency (WADA) and International Olympic Committee in competitive games. Therefore, monitoring the level of propranolol in biological fluids is important for clinical practices and doping control. To ensure the reliability of results obtained from

analytical methods, WADA has established the minimum required performance limit of this drug in urine as 500 g/L [1-5].

There are various methods, such as RP-HPLC-DAD, chromatography, ¹³C NMR spectroscopic and electrochemical method [5-9]. Among all these quantification techniques, electrochemical techniques offered more sensitivity and reliability in sample consumption and miniaturization of the processes [10-17].

Nanotechnology has enormous potential for providing innovative solutions to a wide range of applications [18-23]. The development of nanoscience and nanotechnology has allowed trials to apply different nanomaterials for the fabrication of chemically modified electrodes [24-36]. In recent years, various nanomaterials have been used singly or in composite form to modify electrodes [37-47]. The chemical modification of inert substrate electrodes offers significant advantages in the design and development of electrochemical sensors [48-52]. In operations, the redox-active sites often shuttle electrons between a solution of the analyte and the substrate electrodes, with a significant reduction of the activation overpotential [53-55]. A further advantage of chemically modified electrodes is that they are less prone to surface fouling and oxide formation compared to inert substrate electrodes [56-60].

The carbon paste electrode (CPE) has attracted great attention in electrochemistry due to its non-toxic nature, eco-friendly, low-cost, easy preparation, broad operational potential window, easy chemical and mechanical modification, and renewable surface. Carbon paste is a widely used electrode due to its electrochemical characteristics, such as very low background current, low ohmic resistance, affordability, easy modification and simple renewal of the electrode surface [61-63].

The objective of the present research is the fabrication of a new sensor by modification of a carbon paste electrode with graphene/Co₃O₄ nanocomposite (Gr-Co₃O₄ NC/CPE) for determination of the propranolol. Finally, this technique experienced a successful application for detecting propranolol in the real sample with encouraging outputs.

Experimental

Equipment and materials

In order to do electrochemical tests at ambient temperature, we utilized the Auto-lab potentiostat/galvanostat (PGSTAT 302N, Eco Chemie, the Netherlands) with GPES (General Purpose Electrochemical System-version 4.9) software to control the system. Electrochemical measurements were performed at room temperature in a conventional electrochemical cell with a Gr-Co₃O₄ NC/CPE as the working electrode, 3.0 M Ag/AgCl/KCl as a reference electrode (Azar Electrode, Urmia, Iran) and platinum wire as a counter electrode (Azar Electrode, Urmia, Iran). Moreover, pH was measured using the Metrohm 713 pH meter with a glass electrode (Switzerland). Propranolol and all other solutions used during the procedure were prepared by reagent-grade chemicals from Merck and Sigma-Aldrich and deionized water was supplied from Millipore, Germany.

Preparation of graphene/Co₃O₄ nanocomposite

Firstly, graphene oxide (GO) (20 mg) was dispersed in 20 mL ethanol and ultrasonicated for 30 min. Then, Co(NO₃)₂.6H₂O (0.001 mol) was dissolved in 20 mL ethanol solution and stirred for 30 min at ambient temperature. Subsequently, the prepared two solutions were mixed under stirring and 3.6 mL of ammonia solution (NH₃.H₂O (wt. 25%)) was dropwise added. The mixture was transferred into a Teflon-lined stainless steel autoclave and maintained at 180 °C for 24 h. After completion of the reaction, the product was collected by centrifugation, and washed with deionized water and ethanol. Finally, the graphene/Co₃O₄ nanocomposite was dried at 70 °C overnight in an oven. Figure 1 shows the FE-SEM image of graphene/Co₃O₄ nanocomposite.


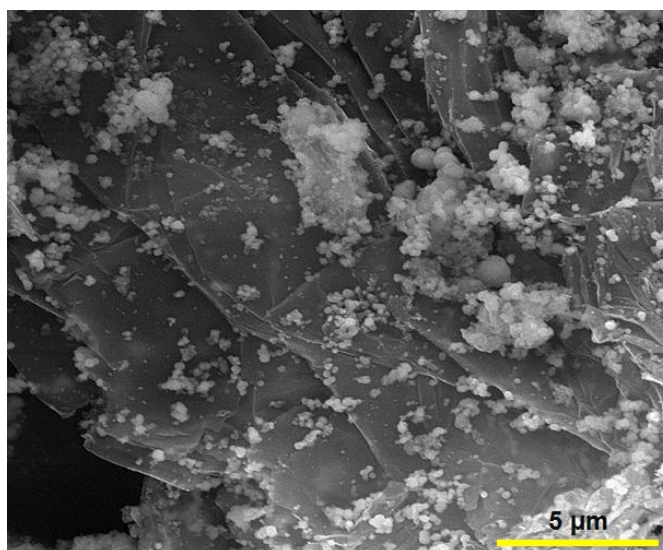


Figure 1. FE-SEM image of graphene/Co₃O₄ nanocomposite.

Preparation and surface modification of electrode

To prepare Gr-Co₃O₄ NC/CPE, 0.95 g graphite powder and 0.05 g graphene/Co₃O₄ nanocomposite were mixed. Next, a suitable amount of paraffin oil was poured into the resulting mixture, followed by mixing well for 30 min to obtain a uniformly wetted paste. An appropriate amount of the paste was tightly packed into a glass tube and a copper wire was positioned over the carbon paste to make electrical contact (Scheme 1).

The surface areas of the Gr-Co₃O₄ NC/CPE and the un-modified CPE were obtained by CV using 1 mM K₃Fe(CN)₆ at various scan rates. Using the Randles–Ševčík equation for Gr-Co₃O₄ NC/CPE, the electrode surface was 0.342 cm², about 3.8 times greater than un-modified CPE.

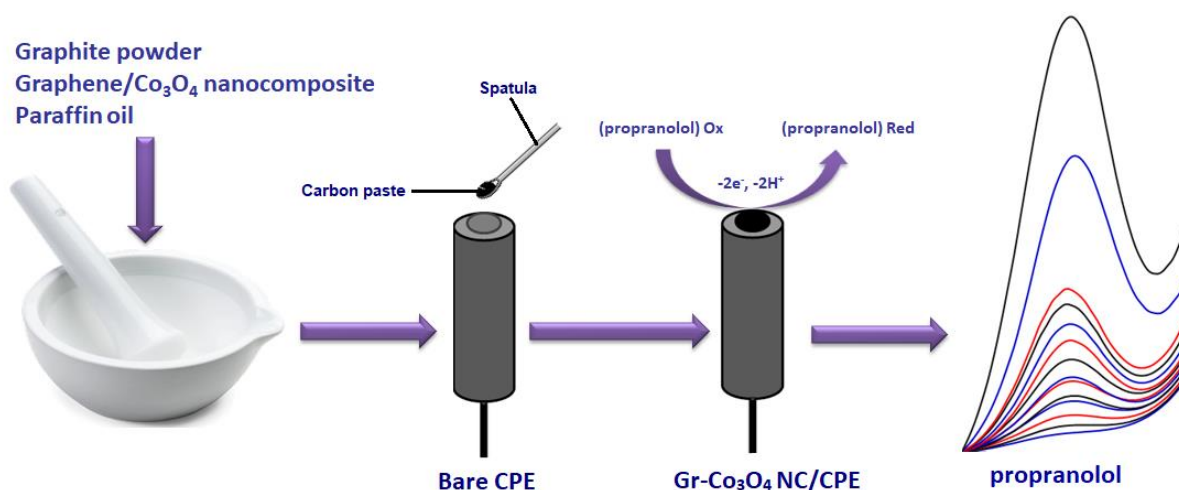

Scheme 1. Scheme of Gr-Co₃O₄ NC/CPE preparation and voltammetric detection of propranolol.

Results and discussion

Electrochemical behavior of propranolol on graphene/Co₃O₄ nanocomposite

The electrochemical behavior of the CPE, Gr-Co₃O₄ NC/CPE was studied by the cyclic voltammetry (CV) technique in the 0.1 M phosphate buffer (pH 7.0) as the supporting electrolyte at a scan rate of 50 mV s⁻¹ (Figure 2). As shown in Figure 2, in comparison to the bare CPE (a), Gr-Co₃O₄ NC/CPE (b) presents a well-defined Irreversible oxide peak with a higher current signal (propranolol concentration equal to 100.0 μM).

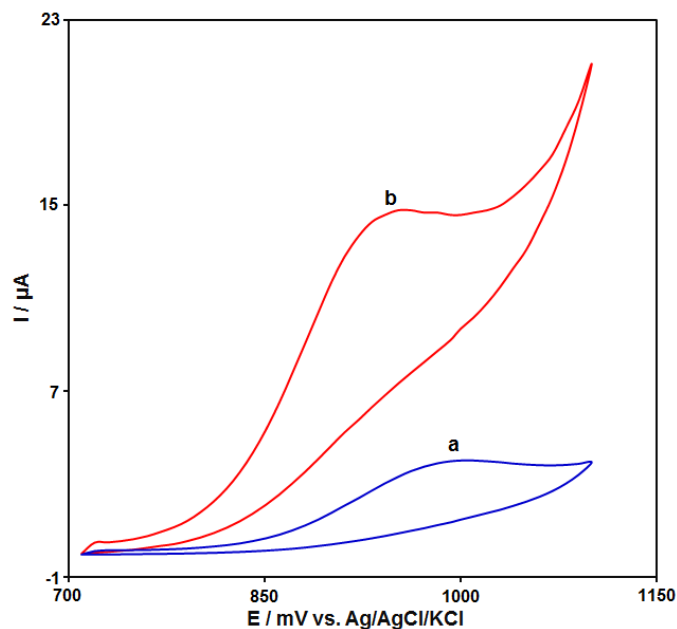


Figure 2. Cyclic voltammograms of a) CPE and b) Gr-Co₃O₄ NC/CPE in the presence of 100.0 μM propranolol at a pH 7.0 of 0.1 M PBS, respectively.

Role of variable scan rates

The effect of the potential scan rates (5-300 mV s⁻¹) on the electrochemical oxidation of propranolol was studied by cyclic voltammetry (CV). Figure 3 shows the CV of 70.0 μM of propranolol in the 0.1 M phosphate buffer solution at the Gr-Co₃O₄ NC/CPE. These results show that the anodic current increases with an increasing scan rate. The oxidation current of propranolol increased linearly with the square root of the scan rate (Figure 3, Inset), which demonstrate a diffusion controlled electrochemical process.

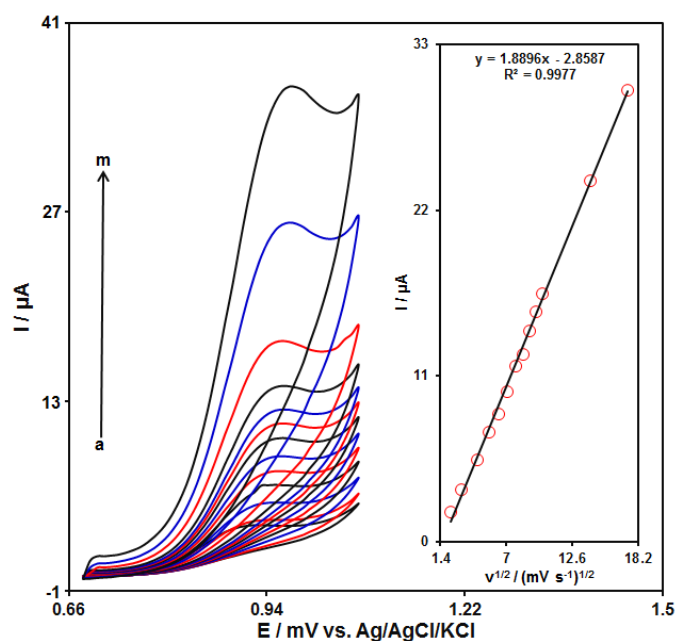


Figure 3. Cyclic voltammograms of propranolol (70.0 μM) at Gr-Co₃O₄ NC/CPE at different scan rates of a) 5, b) 10, c) 20, d) 30, e) 40, f) 50, g) 60, h) 70, i) 80, j) 90 k) 100 l) 200 and m) 300 mV/s in 0.1 M PBS (pH 7.0).
Insert: Plot of I_p versus $v^{1/2}$ for the oxidation of propranolol at Gr-Co₃O₄ NC/CPE.

Chronoamperometric analysis

The chronoamperometric measurements of propranolol at the Gr-Co₃O₄ NC/CPE surface were done to estimate the apparent diffusion coefficient of propranolol under used experimental conditions. Figure 4

shows the current-time profiles obtained by setting the working electrode potential at 1000 mV for different concentrations of propranolol. At long enough experimental times ($t=0.3-3s$), where the electron transfer reaction rate of propranolol is more than its diffusion rate toward the working electrode surface, the current is diffusion controlled. Figure 4, inset A, shows the experimental plots of I versus $t^{-1/2}$ with the best fit for different concentrations of propranolol employed. The slopes of the resulting straight lines were then plotted versus the propranolol concentration (Figure 4, inset B). Based on the Cottrell equation [64], the slope of this plot (Figure 4 inset B) can be used to estimate the apparent diffusion coefficient of propranolol. From the slope of this plot ($29.458 \text{ A s}^{1/2} \text{ mM}^{-1}$), the value of propranolol was found to be $7.4 \times 10^{-5} \text{ cm}^2 \text{ s}^{-1}$ for propranolol.

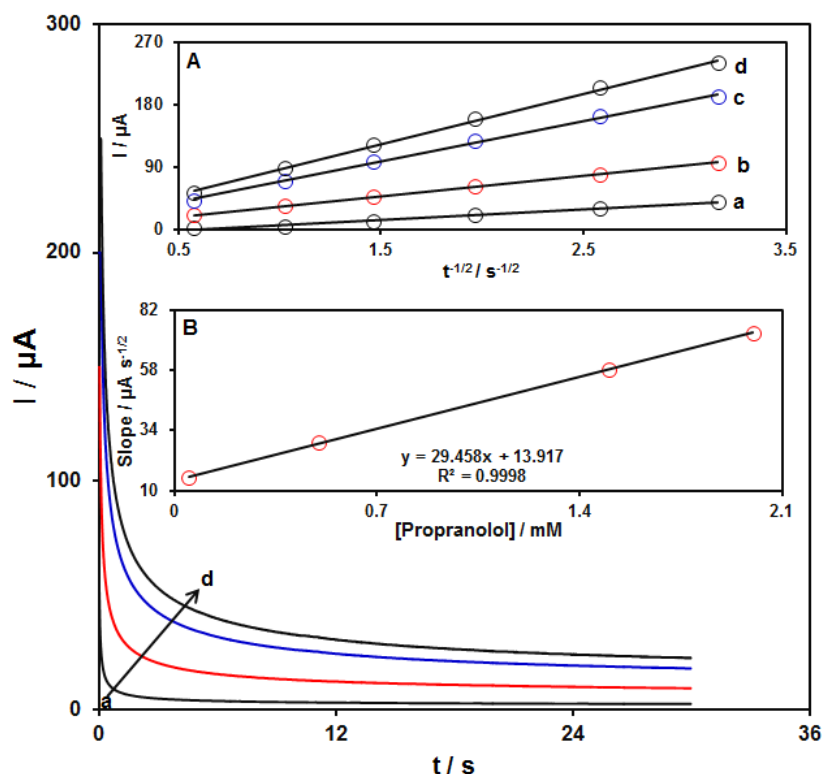


Figure 4. Chronoamperograms obtained at the Gr-Co₃O₄ NC/CPE in the presence of a) 0.05, b) 0.5, c) 1.5 and d) 2.0 mM propranolol in the 0.1 M buffer solution (pH 7.0). A) Plot of I versus $t^{-1/2}$ for electro-oxidation of hydrochlorothiazide obtained from chronoamperograms a–d. B) Plot of slope from straight lines versus propranolol level.

Differential pulse voltammetry analysis of propranolol

Differential pulse voltammetry (DPV) was used for the determination of propranolol at Gr-Co₃O₄ NC/CPE due to its high sensitivity. The DPV responses for different concentrations of propranolol were illustrated in Figure 5 (step potential=0.01 V and pulse amplitude=0.025 V). The linear range was found to be from 1.0 μM to 300.0 μM . The linear equation was $I_p (\mu\text{A}) = 1.6252 + 0.1275 C_{\text{propranolol}} (\mu\text{M})$ with a correlation coefficient of 0.9979. Also, the limit of detection, C_m , of propranolol was calculated using the following equation:

$$C_m = 3S_b/m$$

where, m is the slope of the calibration plot ($0.1275 \mu\text{A}/\mu\text{M}$) and S_b is the standard deviation of the blank response obtained from 10 replicate measurements of the blank solution. The detection limit for the determination of propranolol using this method is $0.3 \mu\text{M}$.

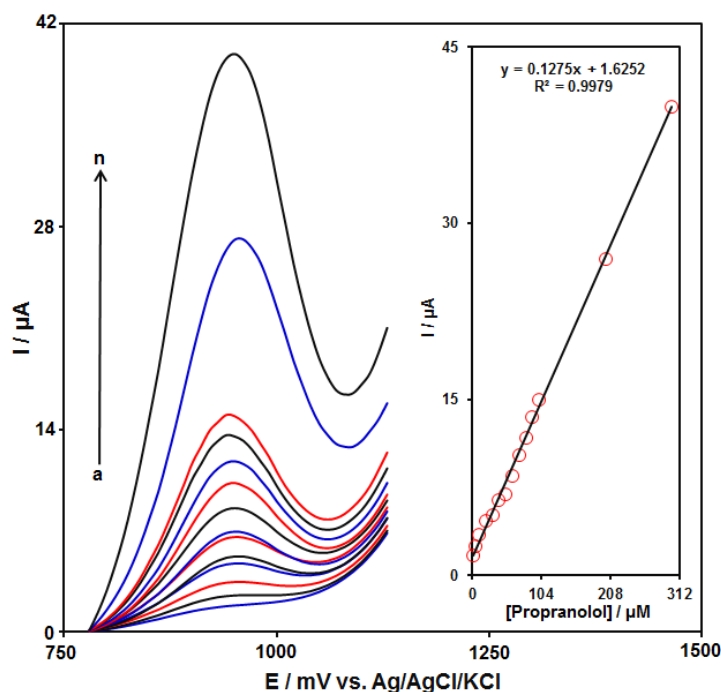


Figure 5. DPV curves of Gr-Co₃O₄ NC/CPE in the 0.1 M buffer solution (pH 7.0) containing different concentrations of propranolol. a-n corresponds to 1.0, 5.0, 10.0, 20.0, 30.0, 40.0, 50.0, 60.0, 70.0, 80.0, 90.0, 100.0, 200.0 and 300.0 μM propranolol. Inset: Plots of electrocatalytic peak current as a function of propranolol concentration.

Conclusion

We arranged a sensor using Gr-Co₃O₄ nanocomposite produced for the detection of propranolol and showed that the results showed the improved behavior of the propranolol sensor with respect to the nanocomposite by s-created. Extensive direct access, limited detection limit (0.3 μM), selectivity and incredible robustness were found for the proposed detection framework as a result of improved properties such as large surface area, fast mass vehicle, remarkable biocompatibility and reactive synergism of Gr-Co₃O₄ nanoparticles. Likewise, the findings recommended Gr-Co₃O₄ NC/CPE nanoparticles as a magnificent sensor for the determination of propranolol.

Conflict of interest: The authors declare no conflict of interest

References

- [1] P. Gupta, S.K. Yadav, B. Agrawal, R.N. Goyal. A novel graphene and conductive polymer modified pyrolytic graphite sensor for determination of propranolol in biological fluids. *Sensors and Actuators B: Chemical* **204** (2014) 791-798. <https://doi.org/10.1016/j.snb.2014.08.040>
- [2] A. Santhy, S. Beena. A study on the recent developments in voltammetric sensors for the β-blocker propranolol hydrochloride. *Biomedical Engineering Applications for People with Disabilities and the Elderly in the COVID-19 Pandemic and Beyond*, (2022) 23-31. <https://doi.org/10.1016/B978-0-323-85174-9.00004-2>
- [3] H. B. Ladmakhi, S. Fathi, F. Chekin, J.B. Raouf. Determination of Propranolol at a Carbon Paste Electrode Modified with Magnetite–Graphene Oxide in Combination with Presence of Sodium Dodecyl Sulfate. *Russian Journal of Electrochemistry* **58(3)** (2022) 184-191. <https://doi.org/10.1134/S1023193522030065>
- [4] M. Yaqub, S. Park, E. Alzahrani, A.E. Farouk, W. Lee. Application of data-driven machine learning to predict propranolol and trimethoprim removal using a managed aquifer recharge system. *Journal of Environmental Chemical Engineering* **10(1)** (2022) 106847. <https://doi.org/10.1016/j.jece.2021.106847>
- [5] M. Khalid, S. Ahmad. Box–Behnken Design Used to Optimize the Simultaneous Quantification of Amitriptyline and Propranolol in Tablet Dosages by RP-HPLC-DAD Method and Their Stability Tests. *Separations* **9(12)** (2022) 421. <https://doi.org/10.3390/separations9120421>

- [6] N.S. Alsultani, A.A. Alkarimi, I.A. Aljazaery. Preparation of Monolithic Chromatographic Column for Propranolol Hydrochloride Determination. *Journal of Pharmaceutical Negative Results* **13(4)** (2022) 1629-1636. <https://doi.org/10.47750/pnr.2022.13.04.226>
- [7] S. Lee, S. Jung. ¹³C NMR spectroscopic analysis on the chiral discrimination of N-acetylphenylalanine, catechin and propranolol induced by cyclic-(1→ 2)-β-d-glucans (cyclosophoraoses). *Carbohydrate research* **337(19)** (2002) 1785-1789. [https://doi.org/10.1016/S0008-6215\(02\)00286-0](https://doi.org/10.1016/S0008-6215(02)00286-0)
- [8] A.M. Santos, A. Wong, O. Fatibello-Filho. Simultaneous determination of salbutamol and propranolol in biological fluid samples using an electrochemical sensor based on functionalized-graphene, ionic liquid and silver nanoparticles. *Journal of Electroanalytical Chemistry* **824** (2018) 1-8. <https://doi.org/10.1016/j.jelechem.2018.07.018>
- [9] M. Khairy, A.A. Khorshed. Simultaneous voltammetric determination of two binary mixtures containing propranolol in pharmaceutical tablets and urine samples. *Microchemical Journal* **159** (2020) 105484. <https://doi.org/10.1016/j.microc.2020.105484>
- [10] H. Karimi-Maleh, F. Karimi, Y. Orooji, G. Mansouri, A. Razmjou, A. Aygun, F. Sen. A new nickel-based co-crystal complex electrocatalyst amplified by NiO dope Pt nanostructure hybrid; a highly sensitive approach for determination of cysteamine in the presence of serotonin. *Scientific Reports* **10(1)** (2020) 1-13. <https://doi.org/10.1038/s41598-020-68663-2>
- [11] A. Lohrasbi-Nejad. Electrochemical strategies for detection of diazinon. *Journal of Electrochemical Science and Engineering* **12(6)** (2022) 1041-1059. <https://doi.org/10.5599/jese.1379>
- [12] H. Beitollahi, S.Z. Mohammadi, M. Safaei, S. Tajik. Applications of electrochemical sensors and biosensors based on modified screen-printed electrodes: a review. *Analytical Methods* **12** (2020) 1547-1560. <https://doi.org/10.1039/C9AY02598G>
- [13] J. Mohanraj, D. Durgalakshmi, R.A. Rakkesh, S. Balakumar, S. Rajendran, H. Karimi-Maleh. Facile synthesis of paper based graphene electrodes for point of care devices: A double stranded DNA (dsDNA) biosensor. *Journal of Colloid and Interface Science* **566** (2020) 463-472. <https://doi.org/10.1016/j.jcis.2020.01.089>
- [14] Y.F. Mustafa, G. Chehardoli, S. Habibzadeh, Z. Arzehgar. Electrochemical detection of sulfite in food samples. *Journal of Electrochemical Science and Engineering* **12(6)** (2022) 1061-1079. <https://doi.org/10.5599/jese.1555>
- [15] M. Mazloun-Ardakani, H. Beitollahi, B. Ganjipour, H. Naeimi. Novel carbon nanotube paste electrode for simultaneous determination of norepinephrine, uric acid and d-penicillamine. *International Journal of Electrochemical Science* **5** (2010) 531-546.
- [16] M. Miraki, H. Karimi-Maleh, M.A. Taher, S. Cheraghi, F. Karimi, S. Agarwal, V.K. Gupta. Voltammetric amplified platform based on ionic liquid/NiO nanocomposite for determination of benserazide and levodopa. *Journal of Molecular Liquids* **278** (2019) 672-676. <https://doi.org/10.1016/j.molliq.2019.01.081>
- [17] M. Velicky, A. N. Rodgers, R.A. Dryfe, K. Tam. Use of voltammetry for in vitro equilibrium and transport studies of ionisable drugs. *ADMET and DMPK* **2(3)** (2014) 143-156. <https://doi.org/10.5599/admet.2.3.22>
- [18] S. Azimi, M. Amiri, H. Imanzadeh, A. Bezaatpour. Fe₃O₄@SiO₂-NH₂/CoSB Modified Carbon Paste Electrode for Simultaneous Detection of Acetaminophen and Chlorpheniramine. *Advanced Journal of Chemistry-Section A* **4(2)** (2021) 152-164. <https://doi.org/10.22034/ajca.2021.275901.1246>
- [19] S. Mahari, S. Gandhi. Electrochemical immunosensor for detection of avian Salmonellosis based on electroactive reduced graphene oxide (rGO) modified electrode. *Bioelectrochemistry* **144** (2022) 108036. <https://doi.org/10.1016/j.bioelechem.2021.108036>
- [20] H. Karimi-Maleh, C. Karaman, O. Karaman, F. Karimi, Y. Vasseghian, L. Fu, M. Baghayeri, J. Rouhi, P. Senthil Kumar, P.L. Show, S. Rajendran. Nanochemistry approach for the fabrication of Fe and N co-decorated biomass-derived activated carbon frameworks: a promising oxygen reduction reaction electrocatalyst in neutral media. *Journal of Nanostructure in Chemistry* **12(3)** (2022) 429-439. <https://doi.org/10.1007/s40097-022-00492-3>

- [21] S. Tajik, M.A. Taher, H. Beitollahi. Simultaneous determination of droxidopa and carbidopa using a carbon nanotubes paste electrode. *Sensors and Actuators B: Chemical* **188** (2013) 923-930. <https://doi.org/10.1016/j.snb.2013.07.085>
- [22] A. Hosseini Fakhrrabad; R. Sanavi Khoshnood; M.R. Abedi; M. Ebrahimi. Fabrication a composite carbon paste electrodes (CPEs) modified with multi-wall carbon nano-tubes (MWCNTs/N, N-Bis (salicyliden)-1,3-propandiamine) for determination of lanthanum (III). *Eurasian Chemical Communications* **3(9)** (2021) 627-634. <http://dx.doi.org/10.22034/ecc.2021.288271.1182>
- [23] M. Yang, Z. Sun, H. Jin, R. Gui. Sulfur nanoparticle-encapsulated MOF and boron nanosheet-ferrocene complex modified electrode platform for ratiometric electrochemical sensing of adriamycin and real-time monitoring of drug release. *Microchemical Journal* **177** (2022) 107319. <https://doi.org/10.1016/j.microc.2022.107319>
- [24] M. Farahmandjou, P. Khalili. ZnO nanoparticles synthesized by co-precipitation method; Morphology and optoelectronic study. *Asian Journal of Green Chemistry* **5(2)** (2021) 219-226. <https://doi.org/10.22034/ajgc.2021.261206.1287>
- [25] H. Beitollahi, S.G. Ivvari, M. Torkzadeh-Mahani. Voltammetric determination of 6-thioguanine and folic acid using a carbon paste electrode modified with ZnO-CuO nanoplates and modifier. *Materials Science and Engineering: C* **69** (2016) 128-133. <https://doi.org/10.1016/j.msec.2016.06.064>
- [26] P.S. Kumar, B.S. Sreeja, K.K. Kumar, G. Padmalaya. Static and dynamic analysis of sulfamethoxazole using GO/ZnO modified glassy carbon electrode by differential pulse voltammetry and amperometry techniques. *Chemosphere* **302** (2022) 134926. <https://doi.org/10.1016/j.chemosphere.2022.134926>
- [27] S.A. Ismaeel; Y.K. Al-Bayati. Determination of trace metformin in pharmaceutical preparation using molecularly imprinted polymer based pvc-membrane. *Eurasian Chemical Communications* **3(11)** (2021) 812-830. <http://dx.doi.org/10.22034/ecc.2021.300477.1224>
- [28] Y. Dessie, S. Tadesse. A Review on Advancements of Nanocomposites as Efficient Anode Modifier Catalyst for Microbial Fuel Cell Performance Improvement, *Journal of Chemical Reviews* **3(4)** (2021) 320-344. <http://dx.doi.org/10.22034/jcr.2021.314327.1128>
- [29] E.C. Martins, E.R. Santana, A. Spinelli. Nitrogen and sulfur co-doped graphene quantum dot-modified electrode for monitoring of multivitamins in energy drinks. *Talanta* **252** (2023) 123836. <https://doi.org/10.1016/j.talanta.2022.123836>
- [30] M. Mazloum-Ardakani, H. Beitollahi, M.K. Amini, F. Mirkhalaf, B.F. Mirjalili, A. Akbari. Application of 2-(3, 4-dihydroxyphenyl)-1, 3-dithialone self-assembled monolayer on gold electrode as a nanosensor for electrocatalytic determination of dopamine and uric acid. *Analyst* **136(9)** (2011) 1965-1970.
- [31] F. Zare Kazemabadi, A. Heydarinasab, A. Akbarzadehkhayavi, M. Ardjmand. Development, Optimization and in vitro Evaluation of Etoposide loaded Lipid Polymer Hybrid Nanoparticles for controlled Drug Delivery on Lung Cancer. *Chemical Methodologies* **5(2)** (2021) 135-152. <https://doi.org/10.22034/chemm.2021.121495>
- [32] S. Wang, H. Wang, S. Liu, H. Guo, J. Meng, M. Chang, S. Wu. Highly sensitive detection of fluoride based on poly (3-aminophenylboronic acid)-reduced graphene oxide multilayer modified electrode. *Food Chemistry* **400** (2023) 134042. <https://doi.org/10.1016/j.foodchem.2022.134042>
- [33] R. Kavade, R. Khanapure, U. Gawali, A. Patil, S. Patil. Degradation of Methyl orange under visible light by ZnO-Polyaniline nanocomposites. *Journal of Applied Organometallic Chemistry* **2(2)** (2022) 101-112. <http://dx.doi.org/10.22034/jaoc.2022.349558.1056>,
- [34] H. Shayegan, V. Safarifard, H. Taherkhani, M.A. Rezvani. Efficient removal of cobalt(II) ion from aqueous solution using amide-functionalized metal-organic framework. *Journal of Applied Organometallic Chemistry* **2(3)** (2022) 109-118. DOI: <http://dx.doi.org/10.22034/jaoc.2022.154718>
- [35] H. Duan, D. Wang, Y. Li. Green chemistry for nanoparticle synthesis. *Chemical Society Reviews* **44(16)** (2015) 5778-5792. <https://doi.org/10.1039/C4CS00363B>
- [36] M. Bijad, A. Hojjati-Najafabadi, H. Asari-Bami, S. Habibzadeh, I. Amini, F. Fazeli. An overview of modified sensors with focus on electrochemical sensing of sulfite in food samples. *Eurasian Chemical Communications* **3(2)** (2021) 116-138. DOI: <http://dx.doi.org/10.22034/ecc.2021.268819.1122>

- [37] M.M. Abdul Hassan, S. Hassan, K.A. Hassan. Green and chemical synthesis of bimetallic nanoparticles (Fe/Ni) supported by zeolite 5A as a heterogeneous Fenton-like catalyst and study of kinetic and thermodynamic reaction for decolorization of reactive red 120 dye from aqueous pollution. *Eurasian Chemical Communications* **4** (2022) 1062-1086. <https://doi.org/10.22034/ecc.2022.342067.1466>
- [38] S. Ariavand, M. Ebrahimi, E. Foladi. Design and Construction of a Novel and an Efficient Potentiometric Sensor for Determination of Sodium Ion in Urban Water Samples. *Chemical Methodologies* **6** (2022) 886-904. <https://doi.org/10.22034/chemm.2022.348712.1567>
- [39] B. Paulchamy, G. Arthi, B.D. Lignesh. A simple approach to stepwise synthesis of graphene oxide nanomaterial. *Journal of Nanomedicine & Nanotechnology* **6(1)** (2015) 1. <https://doi.org/10.4172/-2157-7439.1000253>
- [40] G. Nabi Bidhendi, N. Mehrdadi, M. Firouzbakhsh. Removal of lead from wastewater by iron-benzenetricarboxylate metal-organic frameworks. *Chemical methodologies* **5** (2021) 271-284. <https://doi.org/10.22034/chemm.2021.130208>
- [41] A. Dehno Khalaji, N. Mohammadi, M. Emami. NiO nanoparticles: Synthesis, characterization, and methyl green removal study. *Progress in Chemical and Biochemical Research* **4(4)** (2021) 372-378. <https://doi.org/10.22034/pcbr.2021.294420.1194>
- [42] A. Obaid, S. Al-ghabban, R. Al-Hussain. Appraising Antioxidant and Antibacterial Activities of Zinc Oxide Nanoparticles Synthesized Biologically by Iraqi Propolis. *Chemical Methodologies* **6(5)** (2022) 366-371. <https://doi.org/10.22034/chemm.2022.332390.1448>
- [43] M. Pirozmand, A. Nezhadali, M. Payehghadr, L. Saghatforoush. Ultratrace determination of cadmium ion in petro-chemical sample by a new modified carbon paste electrode as voltammetric sensor. *Eurasian Chemical Communications* **2** (2020) 1021-1032. <https://doi.org/10.22034/ecc.2020.241560.1063>
- [44] S.E. Mousavi Ghahfarokhi, K. Helfi, M. Zargar Shoushtari. Synthesis of the Single-Phase Bismuth Ferrite (BiFeO₃) Nanoparticle and Investigation of Their Structural, Magnetic, Optical and Photocatalytic Properties. *Advanced Journal of Chemistry-Section A* **5(1)** (2022) 45-58. <https://doi.org/10.22034/-ajca.2021.309069.1284>
- [45] L. Qian, S. Durairaj, S. Prins, A. Chen. Nanomaterial-based electrochemical sensors and biosensors for the detection of pharmaceutical compounds. *Biosensors and Bioelectronics* **175** (2021) 112836. <https://doi.org/10.1016/j.bios.2020.112836>
- [46] V. Tallapaneni, L. Mude, D. Pamu, V.V.S.R. Karri. Formulation, characterization and in vitro evaluation of dual-drug loaded biomimetic chitosan-collagen hybrid nanocomposite scaffolds. *Journal of Medicinal and Chemical Sciences* **5** (2022) 1059-1074. <https://doi.org/10.26655/JMCHEMSCI.2022.6.19>
- [47] A. Kannan, S. Radhakrishnan. Fabrication of an electrochemical sensor based on gold nanoparticles functionalized polypyrrole nanotubes for the highly sensitive detection of l-dopa. *Materials Today Communications* **25** (2020) 101330. <https://doi.org/10.1016/j.mtcomm.2020.101330>
- [48] R.M. Mohabis, F. Fazeli, I. Amini, V. Azizkhani. An overview of recent advances in the detection of ascorbic acid by electrochemical techniques. *Journal of Electrochemical Science and Engineering* **12(6)** (2022) 1081-1098. <https://doi.org/10.5599/jese.1561>
- [49] H. Karimi-Maleh, M. Sheikhshoaie, I. Sheikhshoaie, M. Ranjbar, J. Alizadeh, N.W. Maxakato, A. Abbaspourrad. A novel electrochemical epinine sensor using amplified CuO nanoparticles and an-hexyl-3-methylimidazolium hexafluorophosphate electrode. *New Journal of Chemistry* **43(5)** (2019) 2362-2367. <https://doi.org/10.1039/C8NJ05581E>
- [50] A. Meoipun, K. Kaewjua, O. Chailapakul, W. Siangproh. A simple and fast flow injection amperometry for the determination of methimazole in pharmaceutical preparations using an unmodified boron-doped diamond electrode. *ADMET and DMPK* (2023). <https://doi.org/10.5599/admet.1584>
- [51] P.M. Jahani. Flower-like MoS₂ screen-printed electrode based sensor for the sensitive detection of sunset yellow FCF in food samples. *Journal of Electrochemical Science and Engineering* **12(6)** (2022) 1099-1109. <https://doi.org/10.5599/jese.1413>
- [52] S.A. Alavi-Tabari, M.A. Khalilzadeh, H. Karimi-Maleh. Simultaneous determination of doxorubicin and dasatinib as two breast anticancer drugs uses an amplified sensor with ionic liquid and ZnO

- nanoparticle. *Journal of Electroanalytical Chemistry* **811** (2018) 84-88. <https://doi.org/10.1016/j.jelechem.2018.01.034>
- [53] C.M. Brett. Electrochemical impedance spectroscopy in the characterisation and application of modified electrodes for electrochemical sensors and biosensors. *Molecules* **27(5)** (2022) 1497. <https://doi.org/10.3390/molecules27051497>
- [54] S.Z. Mohammadi, F. Mousazadeh, M. Mohammadhasani-Pour. Electrochemical detection of folic acid using a modified screen printed electrode. *Journal of Electrochemical Science and Engineering* **12(6)** (2022) 1111-1120. <https://doi.org/10.5599/jese.1360>
- [55] V. Sanko, A. Şenocak, S. O. Tümay, Y. Orooji, E. Demirbas, A. Khataee. An electrochemical sensor for detection of trace-level endocrine disruptor bisphenol A using Mo₂Ti₂AlC₃ MAX phase/MWCNT composite modified electrode. *Environmental Research* **212** (2022) 113071. <https://doi.org/10.1016/j.envres.2022.113071>
- [56] H. Karimi-Maleh, A.F. Shojaei, K. Tabatabaeian, F. Karimi, S. Shakeri, R. Moradi. Simultaneous determination of 6-mercaptopruine, 6-thioguanine and dasatinib as three important anticancer drugs using nanostructure voltammetric sensor employing Pt/MWCNTs and 1-butyl-3-methylimidazolium hexafluoro phosphate. *Biosensors and Bioelectronics* **86** (2016) 879-884. <https://doi.org/10.1016/j.bios.2016.07.086>
- [57] S. Saghiri, M. Ebrahimi, M. Bozorgmehr. Electrochemical Amplified Sensor with Mgo Nanoparticle and Ionic Liquid: A Powerful Strategy for Methyldopa Analysis. *Chemical Methodologies* **5(3)** (1999) 234-239. <https://doi.org/10.22034/chemm.2021.128530>
- [58] T. Eren, N. Atar, M. L. Yola, H. Karimi-Maleh. a sensitive molecularly imprinted polymer based quartz crystal microbalance nanosensor for selective determination of lovastatin in red yeast rice. *Food chemistry* **185** (2015) 430-436. <https://doi.org/10.1016/j.foodchem.2015.03.153>
- [59] S. Saghiri, M. Ebrahimi, M.R. Bozorgmehr. NiO nanoparticle/1-hexyl-3-methylimidazolium hexafluorophosphate composite for amplification of epinephrine electrochemical sensor. *Asian Journal of Nanosciences and Materials* **4(1)** (2021) 46-52. <https://doi.org/10.26655/AJNANOMAT.2021.1.4>
- [60] H. Karimi-Maleh, R. Darabi, M. Shabani-Nooshabadi, M. Baghayeri, F. Karimi, J. Rouhi, M. Alizadeh, O. Karaman, Y. Vasseghian, C. Karaman. Determination of D&C Red 33 and Patent Blue V Azo dyes using an impressive electrochemical sensor based on carbon paste electrode modified with ZIF-8/g-C₃N₄/Co and ionic liquid in mouthwash and toothpaste as real samples. *Food and Chemical Toxicology* **162** (2022) 112907. <https://doi.org/10.1016/j.fct.2022.112907>
- [61] H. Setiyanto, D. R. Purwaningsih, V. Saraswaty, N. Mufti, M. A. Zulfikar. Highly selective electrochemical sensing based on electropolymerized ion imprinted polyaniline (IIPANI) on a bismuth modified carbon paste electrode (CPE-Bi) for monitoring Nickel (ii) in river water. *RSC Advances* **12(45)** (2022) 29554-29561. <https://doi.org/10.1039/D2RA05196F>
- [62] F. Hosseini, M. Bahmaei, M. Davallo. Electrochemical determination of propranolol, acetaminophen and folic acid in urine, and human plasma using Cu₂O–CuO/rGO/CPE. *Russian Journal of Electrochemistry* **57(4)** (2021) 357-374. <https://doi.org/10.1134/S1023193521040054>
- [63] J. Zoubir, Y. Elkhotfi, C. Radaa, N. Bougdour, A. Idlahcen, I. Bakas, A. Assabbane. Electrocatalytic detection of dimetridazole using an electrochemical sensor Ag@ CPE. Analytical application. Milk, tomato juice and human urine. *Sensors International* **2** (2021) 100105. <https://doi.org/10.1016/j.sintl.2021.100105>
- [64] A. J. Bard, L. R. Faulkner, *Electrochemical Methods: Fundamentals and Applications*, John Wiley & Sons, New York, 2nd edition, 2001.